




Login to the App: Click “Manage Devices”

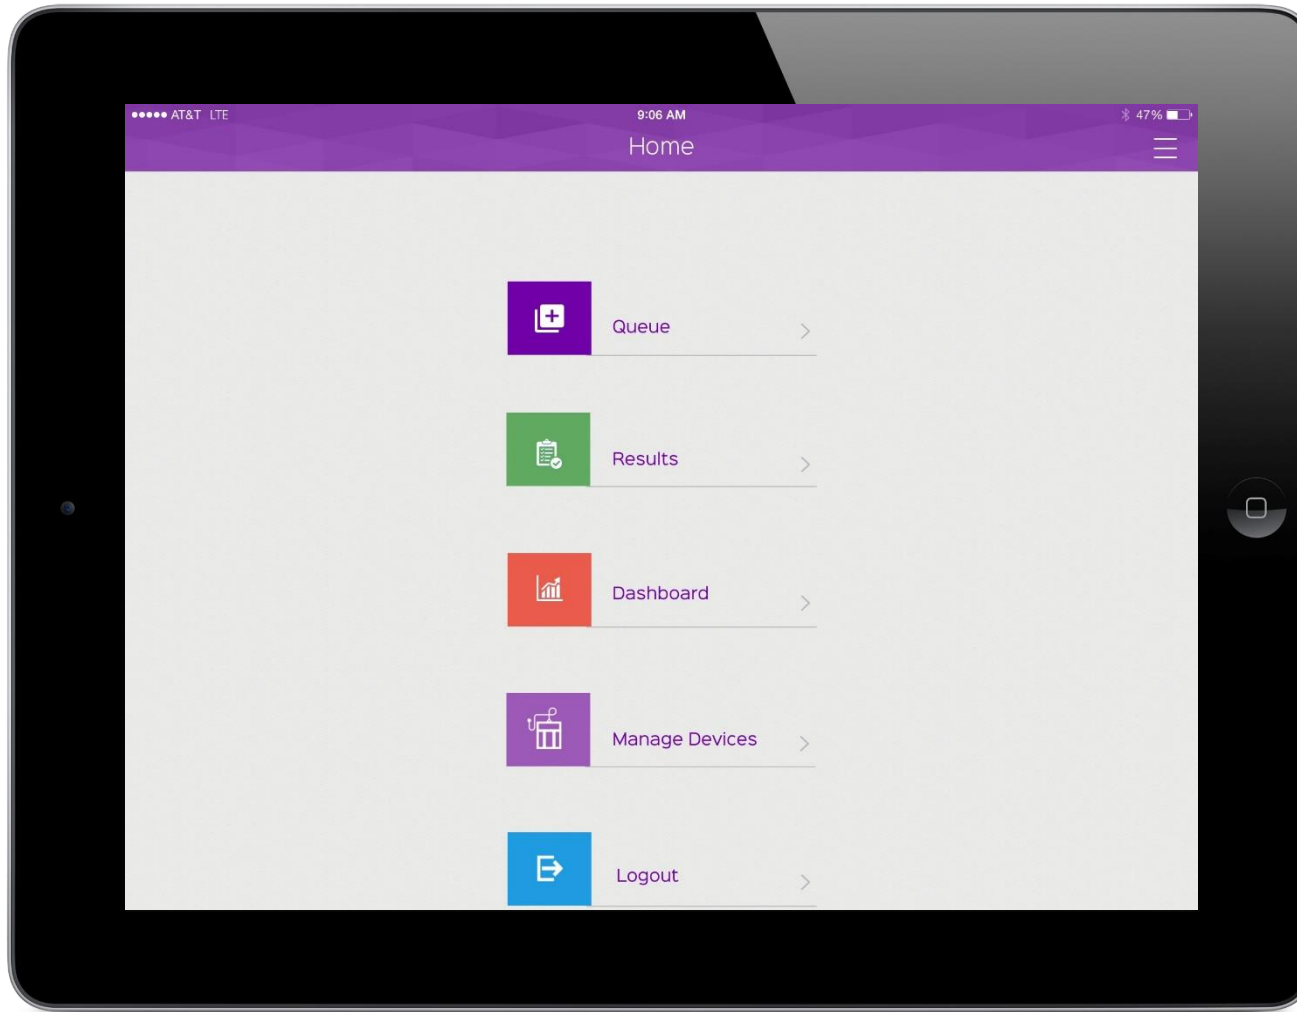


Set Date/Time: Click “Set Date & Time” to proceed

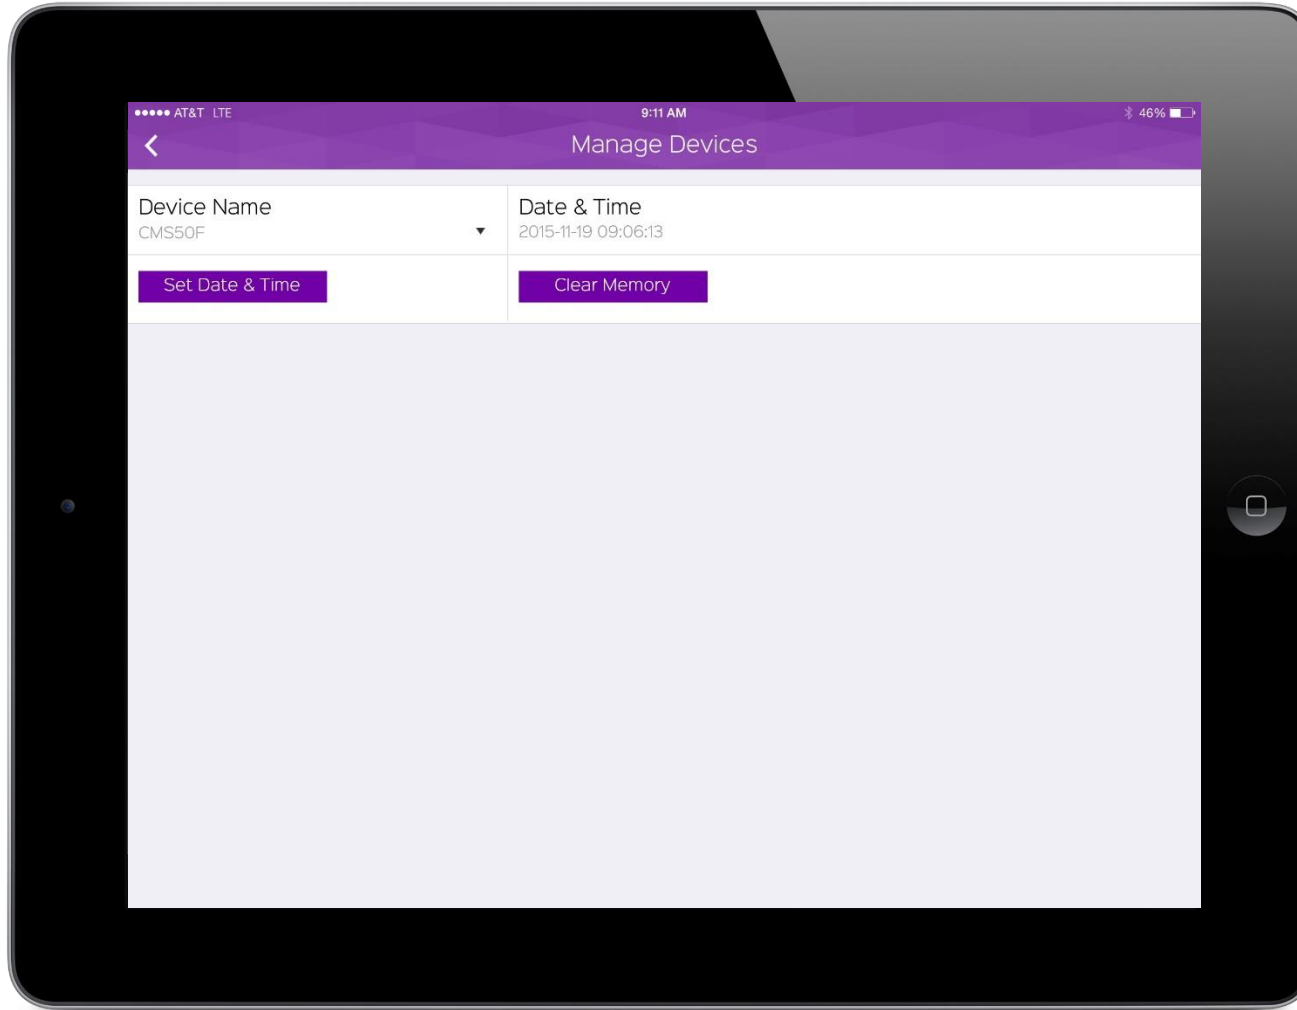

Click “Ok”: Date and Time have been saved to the device

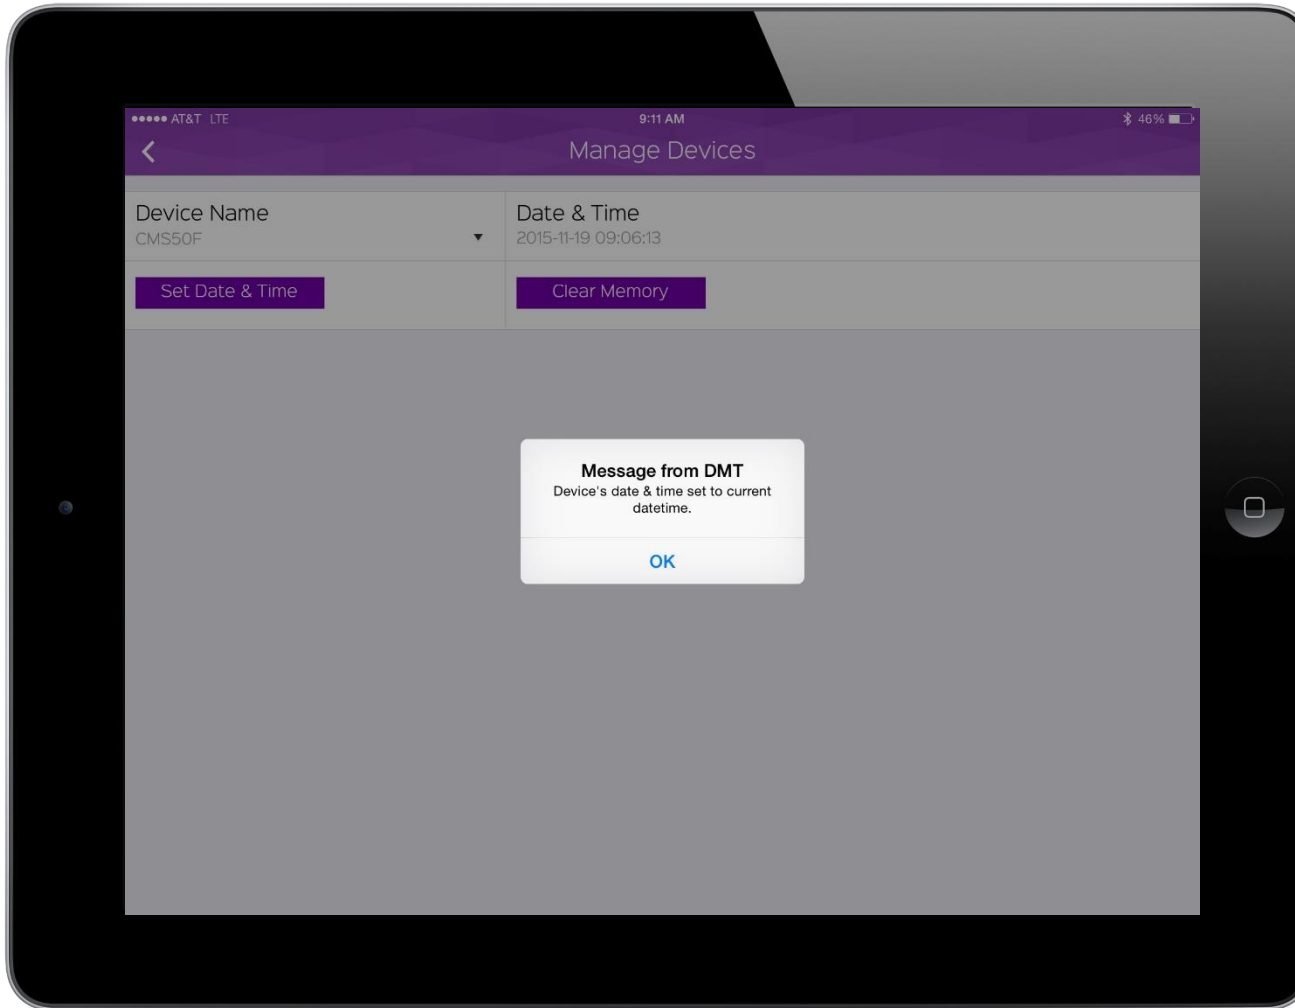

Clear Memory on Device: Click “Clear Memory”

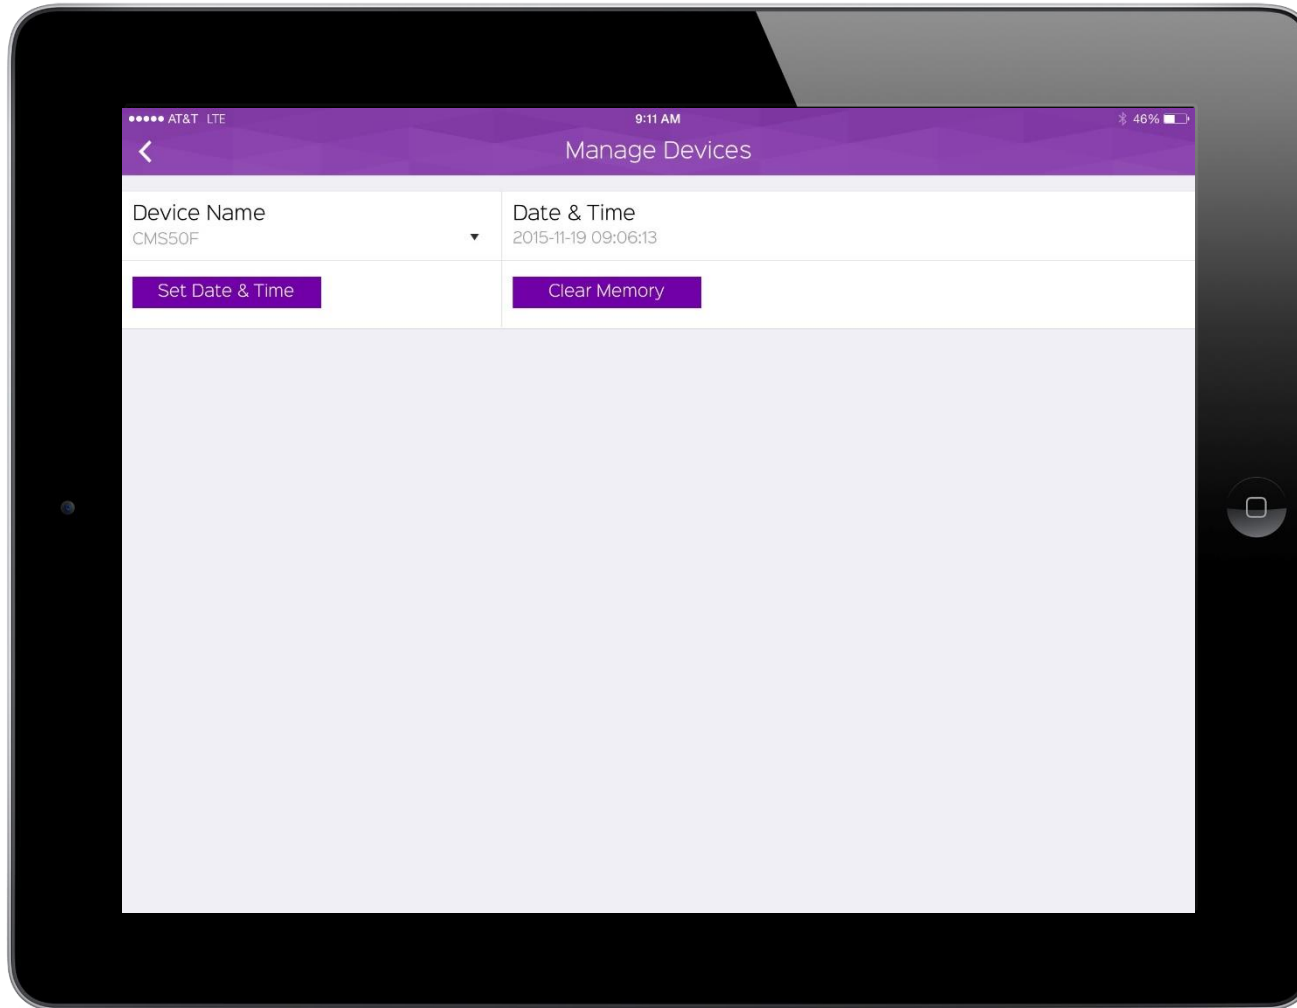

Manage Device via iOS App

Oximeter Used: CMS50F (Only Device to Upload via iOS/Android platform)

Click "Ok": Device Memory has been cleared from the device

